

APPVL INST F100 CRYO ETO 19712 IECE_x
EB-20020486
Revision: AA
Number of Pages: 7
Comments:

THIS COMPONENT MUST COMPLY WITH REGULATORY AGENCY REQUIREMENTS. NO CHANGES ARE ALLOWED WITHOUT PRIOR AUTHORIZATION FROM APPROVALS ENGINEERING.

Originator: RCS 10/13/11

Approved: RCS 10/13/11

Rev	ECN	Description	Approval	Date
AA	1043391	Release to Approvals	RCS	10/13/11



Equipment type **sensor type F100 *****I***** and ETO 19712**

Manufactured and submitted for examination **Micro Motion, Inc.**

Address **Boulder, Co. 80301, USA**

Basis for examination **Annex II of Directive 94/9/EC**

Standard basis IEC 60079-0:2011 General requirements
IEC 60079-11:2011 Intrinsic safety 'i'

Code for type of protection **Ex ib IIC T1 –T6 Gb**


EC Type Examination Certificate **IECEX BVS 11.0090 X**



1) Subject and Type

Sensor type F*** *****|*****

Instead of the *** letters and numerals will be inserted which characterize the following modifications:

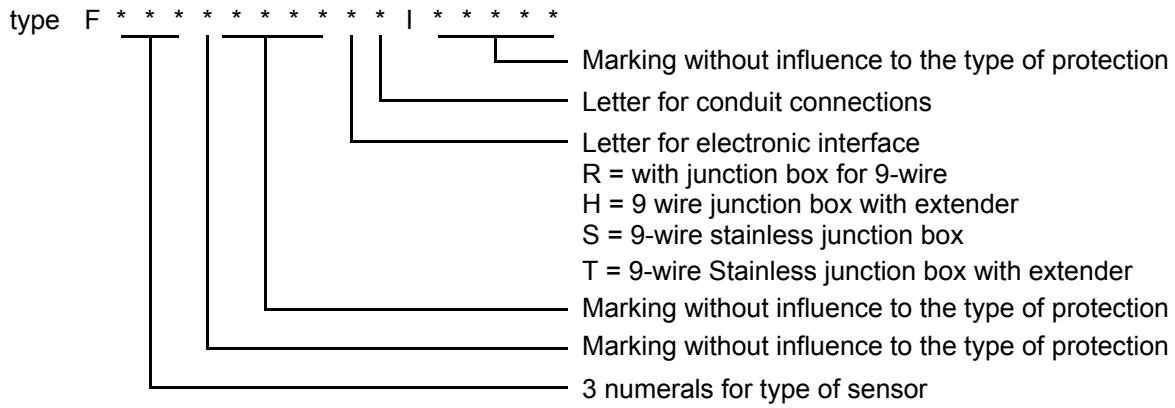


2) Description

The flow sensor in combination with a transmitter is used for flow measurement. The flow sensor, which consists of magnetically excited oscillating tubes, contains as electrical components coils, resistors, temperature sensors and terminals and connectors.

- When used with an integral mounted junction box, the variation gets the denomination F*** *****(S or T)***** for a SS enclosure and F*** *****(R or H)***** for an aluminum enclosure.

Modifications to the design which have impact on the electrical parameters are indicated by a Construction Identification Code (CIC). This code consists out of two digits, starting with an A and followed by a sequence number; for example A4. The CIC can be found on the approval label, see picture below:

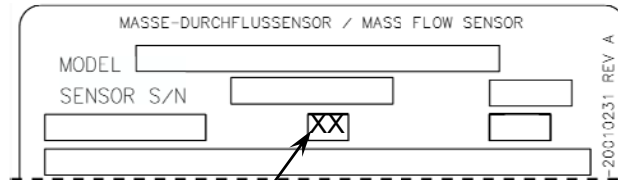


CONSTRUCTION IDENTIFICATION CODE (CIC) (LOCATED APPROXIMATELY WHERE SHOWN)

3) Parameters

3.1. Type F***** (R, H, S or T)***** with J-box and ETO 19712


3.1.1. Drive circuit (connections 1 - 2 or wires red and brown)

Voltage	U _i	DC	11,4	V
Current	I _i		2,45	A
Power	P _i		2,54	W
Effective internal capacitance	C _i		Negligible	

Sensor type		Inductance (mH)	Coil Resistance (Ω)	Series Resistor (Ω)	Minimum Ambient/Fluid Temp (°C)
F100***** (R,H,S,T)***** and ETO 19712	(IIC)	7,5	0	177,2	-40°C/-240°C

3.1.2. Pick-off circuit coil (Terminals 5/9 and 6/8 or wires green/white and blue/grey)

Voltage	U _i	DC	21,13	V
Current	I _i		18,05	mA
Power	P _i		45	mW
Effective internal capacitance	C _i		Negligible	

Sensor type		Inductance (mH)	Coil Resistance (Ω)	Series Resistor (Ω)	Minimum Ambient/Fluid Temp (°C)
F100***** (R,H,S,T)***** and ETO 19712	(IIC)	7,5	0	0-567	-40°C/-240°C



3.1.3. Temperature circuit (terminals 3, 4 and 7 or wires orange, yellow and violet)


Voltage	U _i	DC	21,13	V
Current	I _i		26	mA
Power	P _i		112	mW
Effective internal capacitance	C _i		Negligible	
Effective internal inductance	L _i		Negligible	

3.1.4 Temperature class/ maximum surface temperature T.

The classification into a temperature class/determination of the maximum surface temperature T depends on the temperature of the medium taking into account the maximum operating temperature of the sensor and is shown in the following graphs:

3.1.4.1.

Sensor type		
F100*****(R,H,S,T)*I***** and ETO 19712	(IIC)	Connected to MVD transmitters, e.g. 1000/2000/3000MVD series

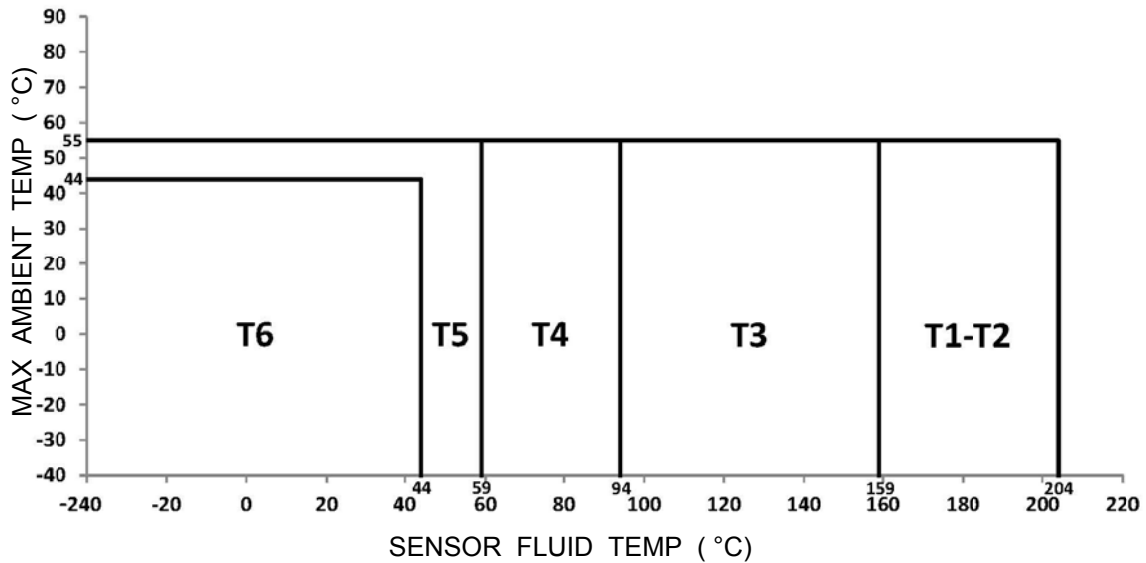

Note 1: Use the above graph to determine the temperature class for a given fluid and ambient temperature.

Ambient temperature range: Ta -40°C to +55°C
 Fluid temperature range: Tm -240°C to +204°C

The use of the sensor at an ambient temperature higher than +55°C is possible, provided that the ambient temperature does not exceed the maximum temperature of the medium taking into account the temperature classification and the maximum operating temperature of the sensor.

4) **Marking**

The marking of the equipment shall include the following:

Type	Type of protection gas	Ambient temperature range
F100***** ¹⁾ I***** and ETO 19712	Ex ib IIC T1-T6 Gb	-40 °C ≤ Ta ≤ +55°C

¹⁾ At this place the letter R, H, S or T will be inserted.